




Islamic Republic of IRAN
Ministry of Health and Medical Education
National Medical Device Directorate

FREE SALES CERTIFICATE


Medical Device

Certificate No: IRI031984
Issue Date: 2024/07/20
Expire Date: 2024/12/04
Product(s): See Attached List
Manufacturer: Hamerz Medical Co. (Sanaye Pezeshki Hamerz)
Address of Manufacturer: Block 36, 1/2 Piece, 4th St, Payam Special Economic Zone, Alborz Province, IRAN

This certificate is hereby issued pursuant to article 81 of the Medical Device Regulation Booklet of I.R.IRAN and the above mentioned Manufacturer complies with the medical device Good Manufacturing Practice (GMP) requirements (Based on ISO 13485).
In conformity with the medical device law of the Islamic Republic of Iran, this product has been registered and is authorized to develop, manufacture and sell in I.R.IRAN and is approved for Export.

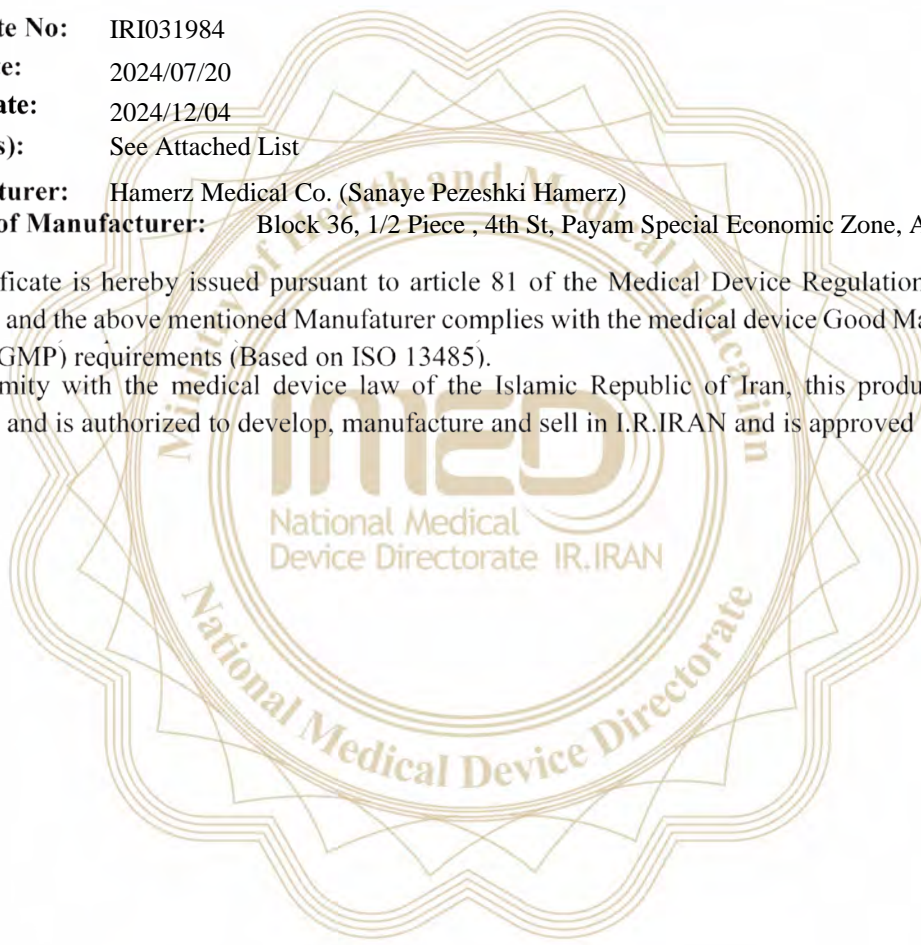

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
& Medical Device Directorate

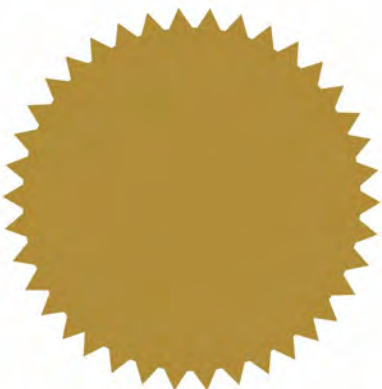



Certificate No : IRI031984
Issue Date : 2024/07/20
Expire Date : 2024/12/04

Row	Name of the device	Model	UMDNS Code	IRC code	IMD code	Use
1	Dental Rotary Instruments	EDGE File	99685	0	29495314	Rotary files is a endodontic
2	Dental Rotary Instruments	EDGE File	99685	921667335 0301698	29495314	Rotary files is a endodontic
3	Dental Rotary Instruments	E-Flex	99685	784364498 4780115	70266897	Rotary files is a endodontic
4	Dental Rotary Instruments	Super Files III	99685	515706365 5539003	31884613	Rotary files is a endodontic

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
&Medical Device Directorate



Islamic Republic of IRAN
Ministry of Health and Medical Education
National Medical Device Directorate

FREE SALES CERTIFICATE

Medical Device

Certificate No: IRI036662
Issue Date: 2024/07/08
Expire Date: 2026/01/20
Product(s): See Attached List
Manufacturer: sanaye pezeshti hamerz
Address of Manufacturer: 36th Block, 1/2 Piece, 4th St, Babaei Blv, Payam Special Economic Zone, Alborz, IRAN

This certificate is hereby issued pursuant to article 81 of the Medical Device Regulation Booklet of I.R.IRAN and the above mentioned Manufacturer complies with the medical device Good Manufacturing Practice (GMP) requirements (Based on ISO 13485).
In conformity with the medical device law of the Islamic Republic of Iran, this product has been registered and is authorized to develop, manufacture and sell in I.R.IRAN and is approved for Export.

Dr. SaeedReza Shahmoradi

Chief Executive of the Equipment
& Medical Device Directorate





Certificate No : IRI036662
Issue Date : 2024/07/08
Expire Date : 2026/01/20

Row	Name of the device	Model	UMDNS Code	IRC code	IMD code	Use
1	Composite	Single tube composite	16724	160670369 6522150	18499934	Restorative consumption/
2	Composite	Single tube composite	16724	490219782 6807423	23190594	Restorative consumption/
3	Composite	Single tube composite	16724	586248396 3359519	56041431	Restorative consumption/
4	Composite	Single tube composite	16724	144956424 1429640	62986534	Restorative consumption/

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
& Medical Device Directorate




Islamic Republic of IRAN
Ministry of Health and Medical Education
National Medical Device Directorate

FREE SALES CERTIFICATE


Medical Device

Certificate No: IRI036469
Issue Date: 2024/07/20
Expire Date: 2026/02/27
Product(s): See Attached List
Manufacturer: Hamerz Medical Co. (Sanaye Pezeshki Hamerz)
Address of Manufacturer: Block 36, 1/2 Piece, 4th St, Payam Special Economic Zone, Alborz Province, IRAN

This certificate is hereby issued pursuant to article 81 of the Medical Device Regulation Booklet of I.R.IRAN and the above mentioned Manufacturer complies with the medical device Good Manufacturing Practice (GMP) requirements (Based on ISO 13485).
In conformity with the medical device law of the Islamic Republic of Iran, this product has been registered and is authorized to develop, manufacture and sell in I.R.IRAN and is approved for Export.

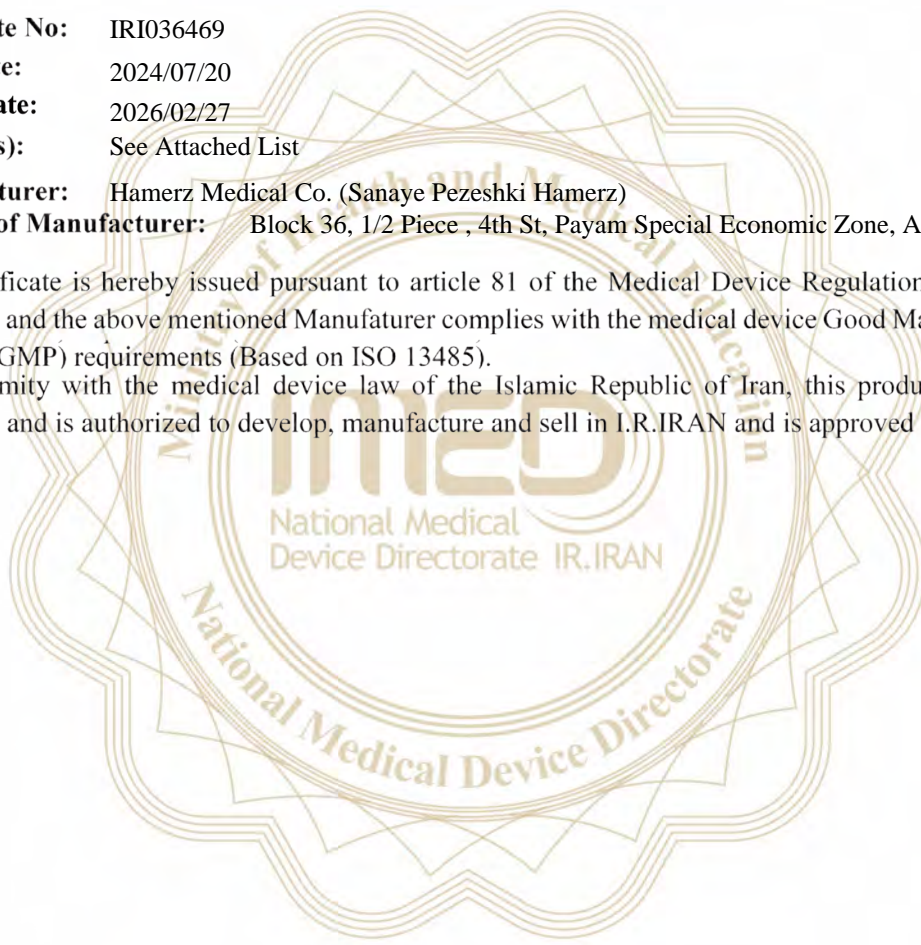

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
& Medical Device Directorate

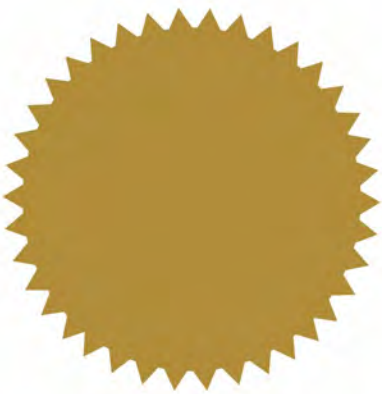



Certificate No : IRI036469
Issue Date : 2024/07/20
Expire Date : 2026/02/27

Row	Name of the device	Model	UMDNS Code	IRC code	IMD code	Use
1	Porcelain Etchant	Porcelainetchant	99713	974672275 3626391	81913194	Porcelain H acid (10% hydrofluoric

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
&Medical Device Directorate




Islamic Republic of IRAN
Ministry of Health and Medical Education
National Medical Device Directorate

FREE SALES CERTIFICATE


Medical Device

Certificate No: IRI039773
Issue Date: 2024/07/22
Expire Date: 2026/03/14
Product(s): See Attached List
Manufacturer: Hamerz Medical Co. (Sanaye Pezeshki Hamerz)
Address of Manufacturer: Block 36, 1/2 Piece, 4th St, Payam Special Economic Zone, Alborz Province, IRAN

This certificate is hereby issued pursuant to article 81 of the Medical Device Regulation Booklet of I.R.IRAN and the above mentioned Manufacturer complies with the medical device Good Manufacturing Practice (GMP) requirements (Based on ISO 13485).
In conformity with the medical device law of the Islamic Republic of Iran, this product has been registered and is authorized to develop, manufacture and sell in I.R.IRAN and is approved for Export.

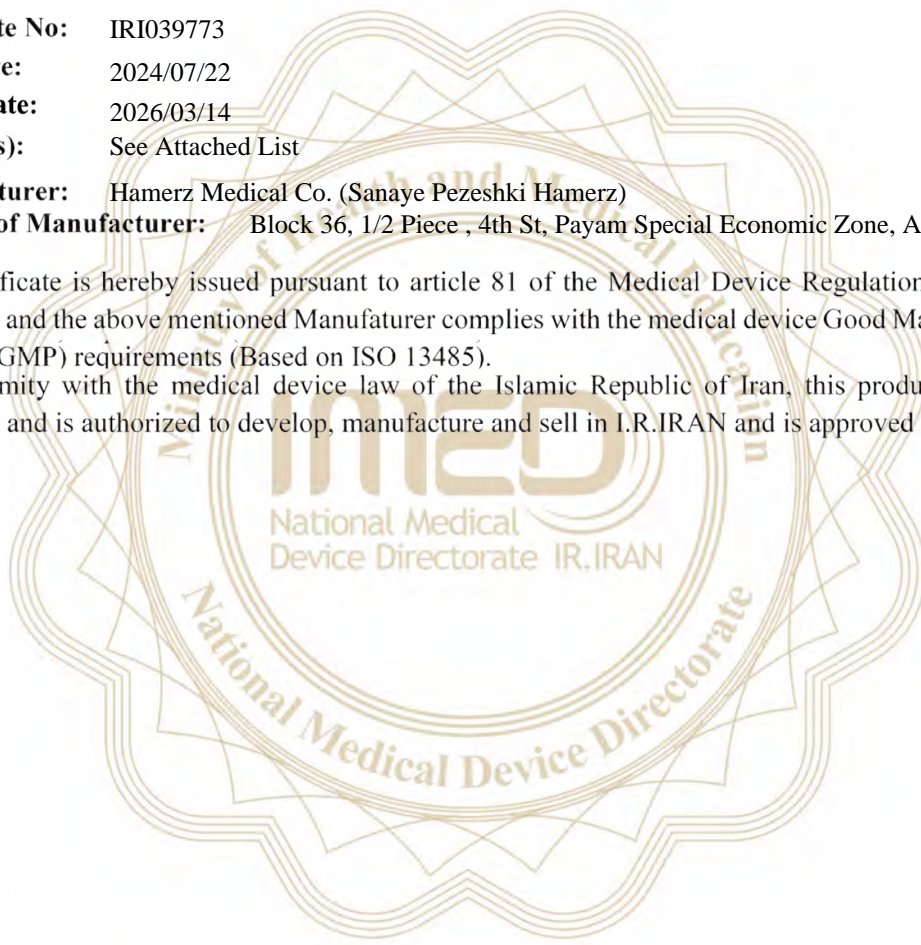

Dr. Saeed Reza Shahmoradi
Chief Executive of the Equipment
& Medical Device Directorate

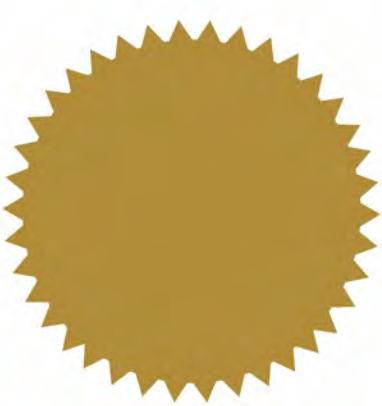



Certificate No : IRI039773
Issue Date : 2024/07/22
Expire Date : 2026/03/14

Row	Name of the device	Model	UMDNS Code	IRC code	IMD code	Use
1	Bonding	Edge Bond SE	99854	844421427 4255415	71458720	Adhesive Resin for dental
2	Bonding	Edge Bond	99854	975037643 8741121	92837817	Adhesive Resin for dental

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
&Medical Device Directorate




Islamic Republic of IRAN
Ministry of Health and Medical Education
National Medical Device Directorate

FREE SALES CERTIFICATE


Medical Device

Certificate No: IRI036765
Issue Date: 2024/07/23
Expire Date: 2026/05/21
Product(s): See Attached List
Manufacturer: Hamerz Medical Co. (Sanaye Pezeshki Hamerz)
Address of Manufacturer: Block 36, 1/2 Piece, 4th St, Payam Special Economic Zone, Alborz Province, IRAN

This certificate is hereby issued pursuant to article 81 of the Medical Device Regulation Booklet of I.R.IRAN and the above mentioned Manufacturer complies with the medical device Good Manufacturing Practice (GMP) requirements (Based on ISO 13485).
In conformity with the medical device law of the Islamic Republic of Iran, this product has been registered and is authorized to develop, manufacture and sell in I.R.IRAN and is approved for Export.

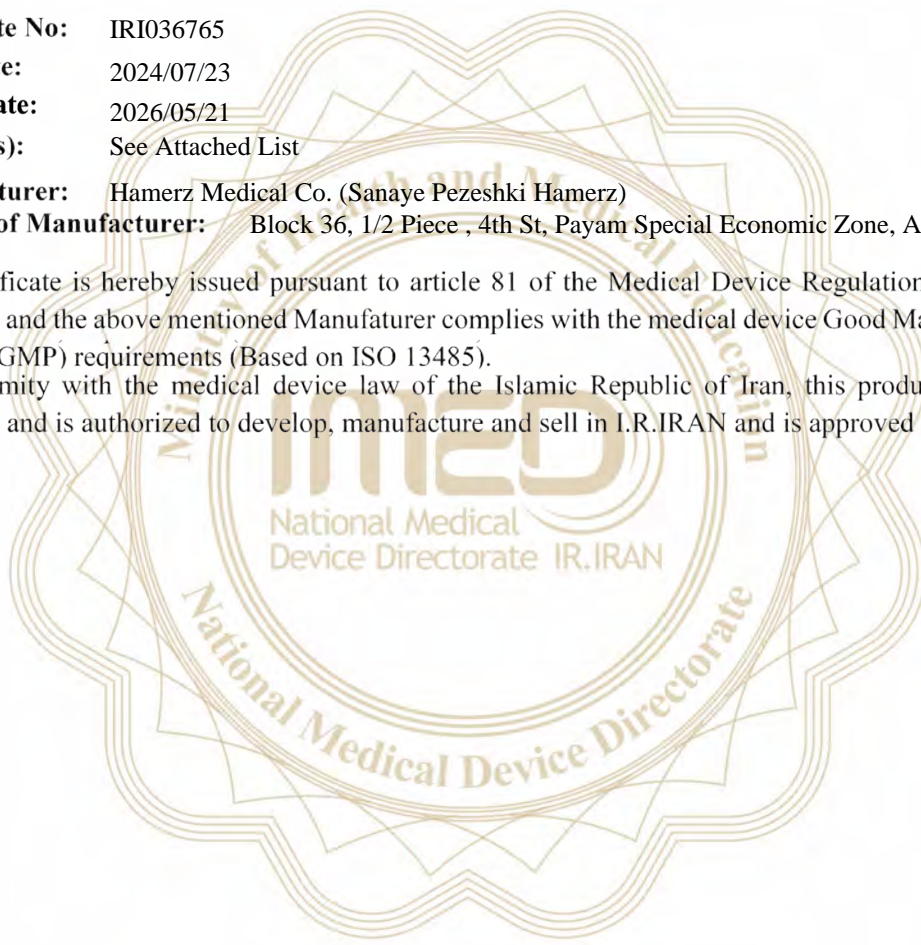

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
& Medical Device Directorate

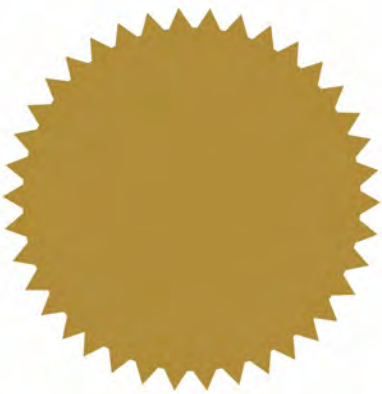



Certificate No : IRI036765
Issue Date : 2024/07/23
Expire Date : 2026/05/21

Row	Name of the device	Model	UMDNS Code	IRC code	IMD code	Use
1	Bleaching Gel	Edge White	99967	668091363 9864237	78459432	dental whitening agents

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
&Medical Device Directorate



Islamic Republic of IRAN
Ministry of Health and Medical Education
National Medical Device Directorate

FREE SALES CERTIFICATE

Medical Device

Certificate No: IRI038231
Issue Date: 2024/07/22
Expire Date: 2026/02/26
Product(s): See Attached List
Manufacturer: Hamerz Medical Co. (Sanaye Pezeshki Hamerz)
Address of Manufacturer: Block 36, 1/2 Piece, 4th St, Payam Special Economic Zone, Alborz Province, IRAN

This certificate is hereby issued pursuant to article 81 of the Medical Device Regulation Booklet of I.R.IRAN and the above mentioned Manufacturer complies with the medical device Good Manufacturing Practice (GMP) requirements (Based on ISO 13485).
In conformity with the medical device law of the Islamic Republic of Iran, this product has been registered and is authorized to develop, manufacture and sell in I.R.IRAN and is approved for Export.

Dr. Saeed Reza Shahmoradi
Chief Executive of the Equipment
& Medical Device Directorate





Certificate No : IRI038231
Issue Date : 2024/07/22
Expire Date : 2026/02/26

Row	Name of the device	Model	UMDNS Code	IRC code	IMD code	Use
1	RC-Prep	Hamerz RC-Prep	99850	695197688 1600747	12489776	EDTA material to lubricate

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
&Medical Device Directorate



Islamic Republic of IRAN
Ministry of Health and Medical Education
National Medical Device Directorate

FREE SALES CERTIFICATE

Medical Device

Certificate No: IRI034892
Issue Date: 2024/07/21
Expire Date: 2026/03/03
Product(s): See Attached List
Manufacturer: Hamerz Medical Co. (Sanaye Pezeshki Hamerz)
Address of Manufacturer: Block 36, 1/2 Piece, 4th St, Payam Special Economic Zone, Alborz Province, IRAN

This certificate is hereby issued pursuant to article 81 of the Medical Device Regulation Booklet of I.R.IRAN and the above mentioned Manufacturer complies with the medical device Good Manufacturing Practice (GMP) requirements (Based on ISO 13485).
In conformity with the medical device law of the Islamic Republic of Iran, this product has been registered and is authorized to develop, manufacture and sell in I.R.IRAN and is approved for Export.

Dr. Saeed Reza Shahmoradi
Chief Executive of the Equipment
& Medical Device Directorate





Certificate No : IRI034892
Issue Date : 2024/07/21
Expire Date : 2026/03/03

Row	Name of the device	Model	UMDNS Code	IRC code	IMD code	Use
1	EDTA	HAMERZEDTA	99694	126244632 7673858	93852893	To simplify the instrumental
2	EDTA	HAMERZEDTA	99694	126244632 7673858	93852893	To simplify the instrumental

Dr. SaeedReza Shahmoradi
Chief Executive of the Equipment
&Medical Device Directorate